


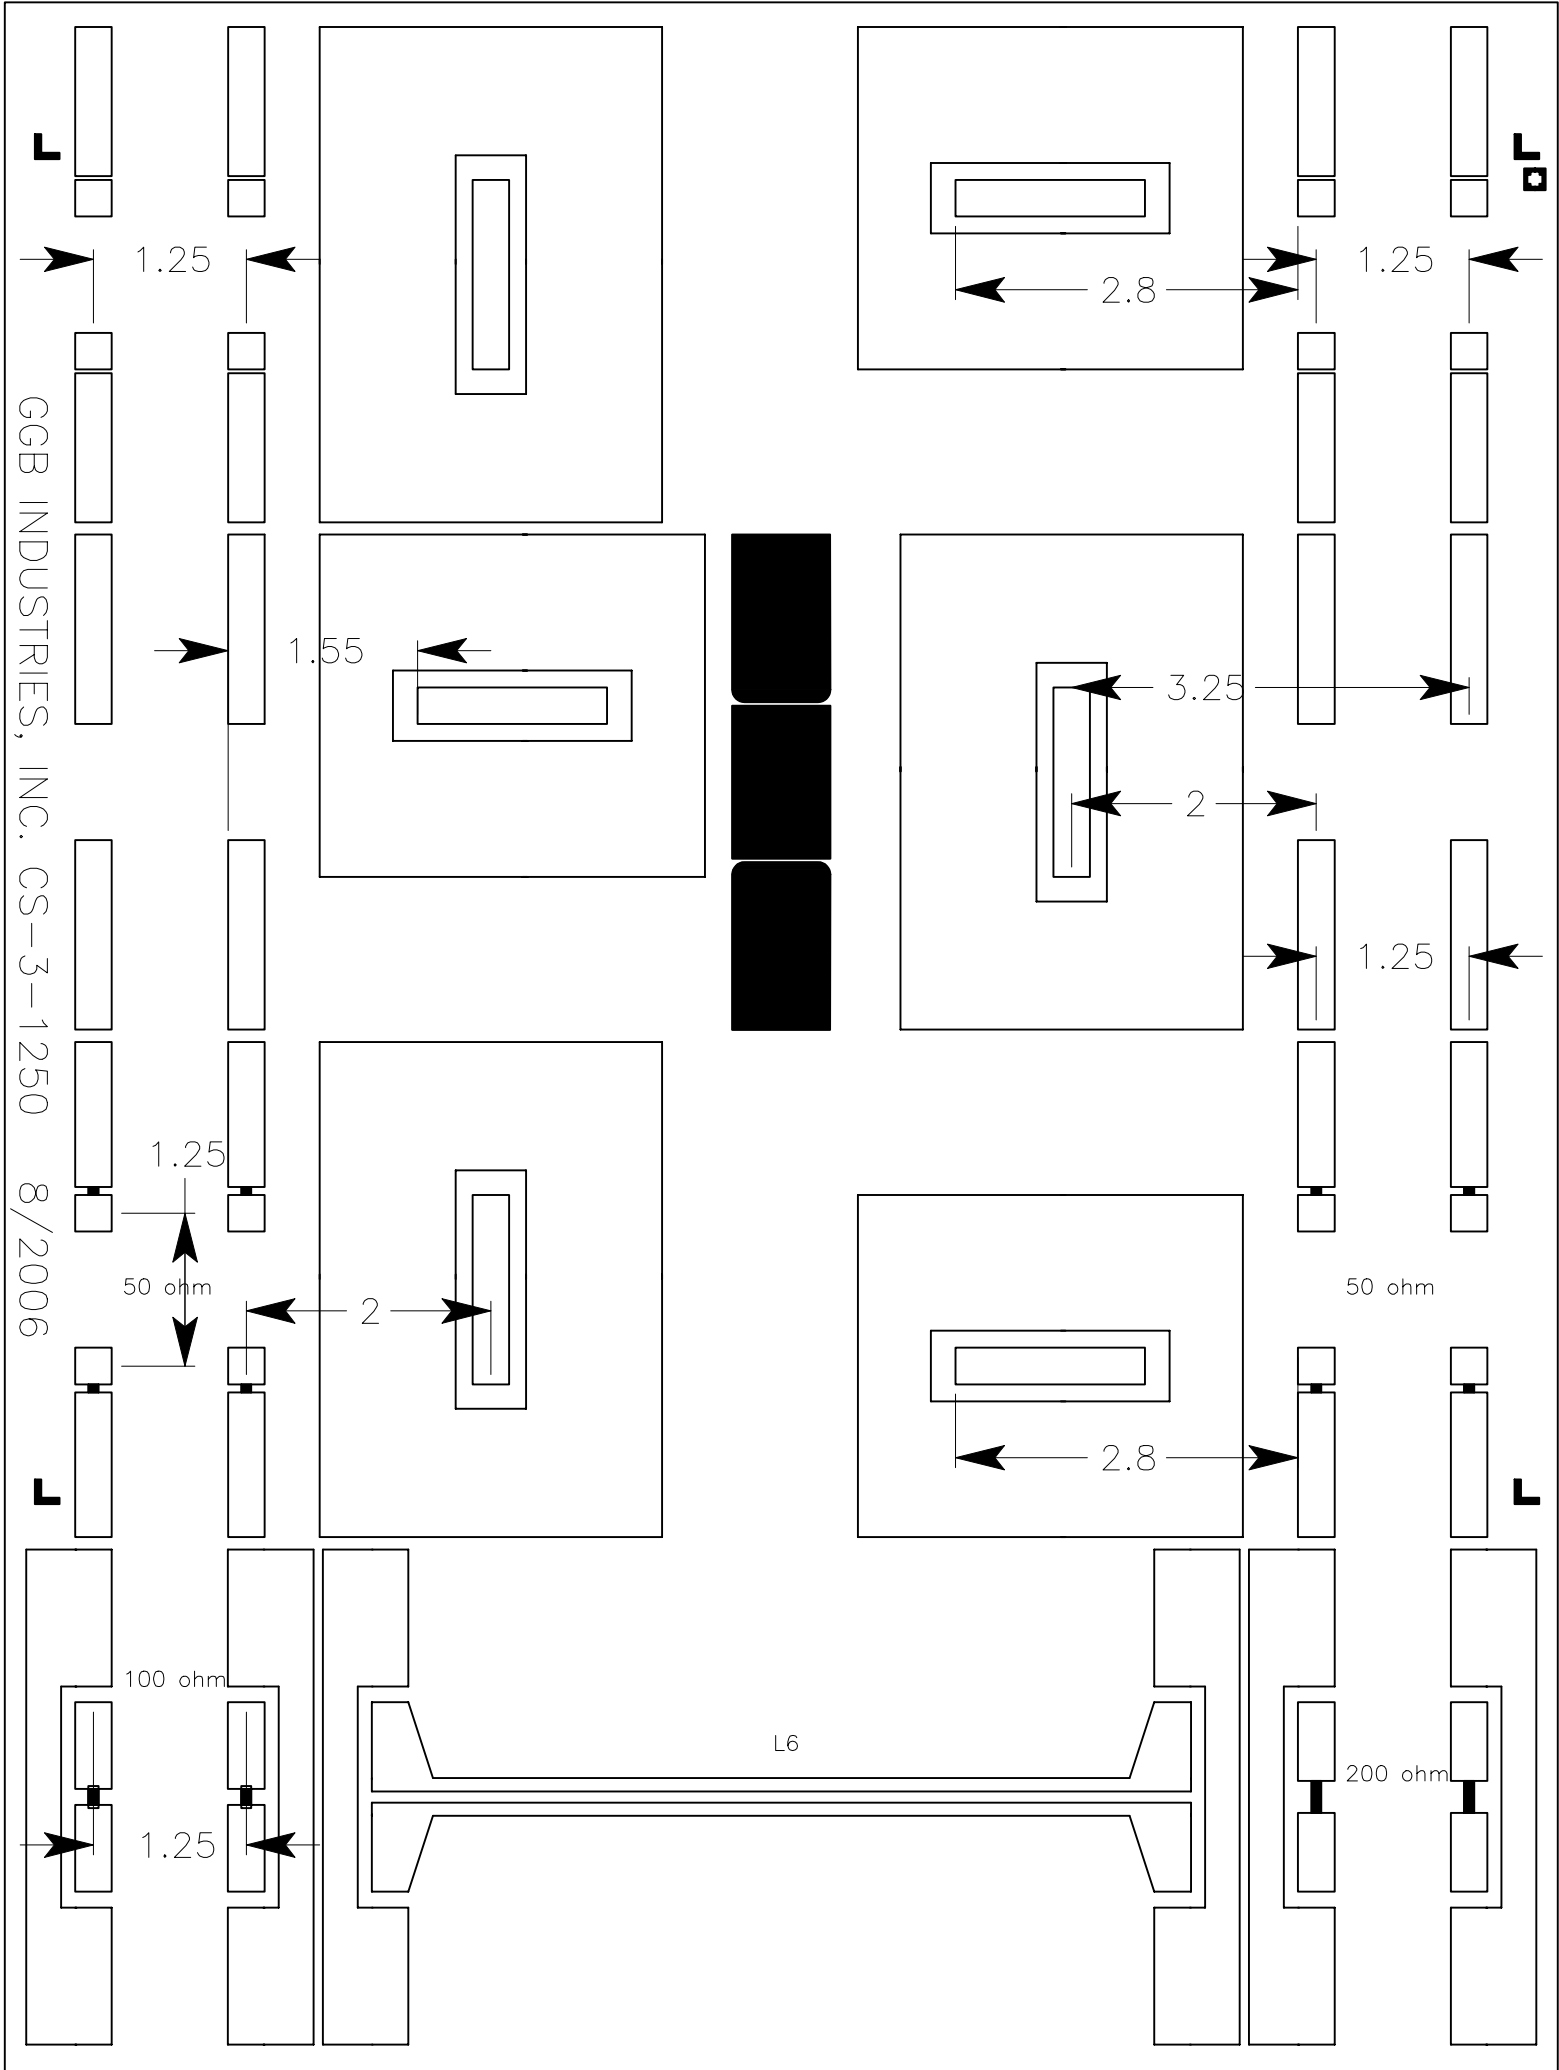

GGB INDUSTRIES, INC. CS-3-1250 8/2006

L6

CS-3-1250 Calibration Substrate Key

(Table 1)

(all structures for GSSG probes)

Location #	Description
10-15	Thrus
1-2	Opens
3-4	Shorts
5-6	50 ohm loads
7	100 ohm structure
8	200 ohm structure
16	6700 micron long balanced verification line